

High-Sensitivity Gas-Pressure Sensor Based on Fiber-Tip PVC Diaphragm Fabry–Pérot Interferometer

Zhe Zhang, Changrui Liao, Jian Tang, Zhiyong Bai, Kuikui Guo, Maoxiang Hou, Jun He, Ying Wang, Shen Liu, Feng Zhang, and Yiping Wang, *Senior Member, IEEE*

Abstract—We demonstrate a novel polyvinyl chloride (PVC) diaphragm-based fiber-tip Fabry–Pérot interferometer for gas-pressure measurements with ultrahigh sensitivity. The PVC diaphragm has been coated to the end facet of a well-cut standard single-mode fiber by use of a plastic welder. An ultrahigh-pressure sensitivity of ~ 65.5 nm/MPa at 1565 nm and a low-temperature cross sensitivity of ~ -5.5 kPa/°C have been experimentally demonstrated. The proposed sensor has advantages of high pressure sensitivity, miniature size, low cost, and easy fabrication.

Index Terms—Optical fiber devices, optical fiber measurements, thin-film devices.

I. INTRODUCTION

FIBER-OPTIC Fabry–Pérot interferometers (FPIs) have advantages such as immunity to electromagnetic interference, miniature size, and the capability of taking probe-type measurements, making it a good candidate for many applications in biomedicine, artificial intelligence, and environmental monitoring. Various FPI sensors have been proposed and applied for measurements of strain [1], refractive index [2], [3], vibration [4], temperature [3], [5]–[8], pressure [9]–[15], and acoustic signal [16]–[18]. Among them, FPI-tip pressure sensors employing an elastic diaphragm at the fiber tip as one of the reflecting mirrors have attracted tremendous research interest. The elastic diaphragm may be composed of polymer [9], [19], silica [10], [20], silver [12], graphene [15], or even water film [13]. Polymer

Manuscript received March 12, 2017; revised May 24, 2017; accepted May 28, 2017. Date of publication May 30, 2017; date of current version August 7, 2017. This work was supported in part by the National Natural Science Foundation of China under Grant 61635007, Grant 61425007, Grant 61377090, Grant 61575128, and Grant 61675137, in part by the Guangdong Natural Science Foundation under Grant 2014A030308007, Grant 2014B050504010, Grant 2015B010105007, and Grant 2015A030313541, in part by the Science and Technology Innovation Commission of Shenzhen under Grant GJHZ20150313093755757, Grant JCYJ20160520163134575, and Grant JCYJ20160427104925452, and in part by the Pearl River Scholar Fellowships. (Corresponding authors: Changrui Liao; Yiping Wang.)

The authors are with the Key Laboratory of Optoelectronic Devices and Systems of Ministry of Education and Guangdong Province, College of Optoelectronic Engineering, Shenzhen University, Shenzhen 518060, China (e-mail: 2150190115@email.szu.edu.cn; cliao@szu.edu.cn; tangjian2@email.szu.edu.cn; bzy041217@126.com; 2150190116@email.szu.edu.cn; maoxiangh@szu.edu.cn; hejun07@szu.edu.cn; yingwang@szu.edu.cn; liushen.szu@gmail.com; zhangfeng840401@gmail.com; ypwang@szu.edu.cn).

Color versions of one or more of the figures in this paper are available online at <http://ieeexplore.ieee.org>.

Digital Object Identifier 10.1109/JLT.2017.2710210

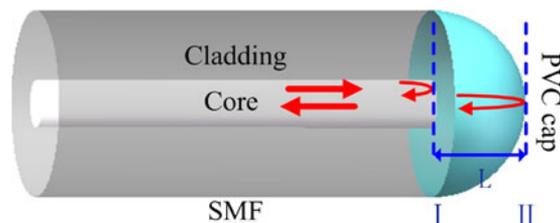


Fig. 1. Schematic of the proposed fiber-tip FPI.

materials with the advantages of versatility, easy fabrication, and low-cost processing have been considered an excellent choice for optical sensor structures. A low elastic modulus can provide adequate sensitivity for polymer-based FPI pressure sensors. Usually, the polymer tip of the FPI is fabricated using conventional semi-conduction processes such as photolithography, chemical vapor deposition (CVD), and/or reactive-ion etching (RIE) on wafer scale [21], [22], or by use of dip coating [16], [23] or ultraviolet (UV) curing adhesive [9], [18], [24] methods. However, all of the aforementioned fabrication methods are complicated and the pressure sensitivities achieved are not high enough.

In this Letter, a novel method of fabricating ultrasensitive FPI pressure sensors is experimentally demonstrated. The proposed probe-type sensing structure is miniaturized and based on a **polyvinyl chloride** (PVC) cap created on the end facet of a standard single-mode fiber (SMF). The pressure sensitivity of the proposed sensor at 1565 nm is ~ 65.5 nm/MPa, which is ~ 60 times higher than reported in our previous work [24], and the temperature cross-sensitivity is ~ 5.5 kPa/°C, which is ~ 40 times lower than that reported in [24]. Moreover, the proposed fabrication method is highly efficient, low cost, and repeatable, and employs only a fiber cleaver and a plastic welder.

II. SENSOR FABRICATION

Fig. 1 is a schematic of the proposed fiber-tip FPI. A few layers of commercial PVC diaphragm are folded together (multilayer PVC diaphragm) and welded to the end facet of a well-cut SMF by use of a plastic welder. In this process, the PVC diaphragms fused and solidified, forming a PVC cap on the end facet of the SMF. Two reflected waves are collected and transmitted back to the SMF: one is from the interface between the fiber end

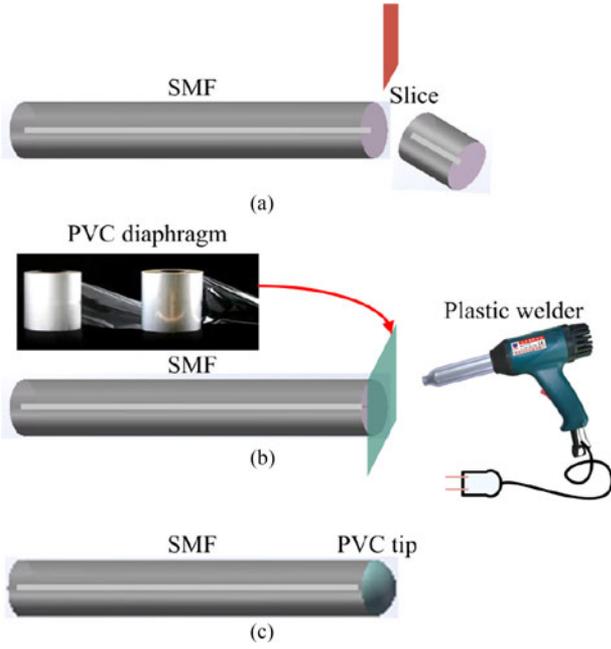


Fig. 2. Schematic of the fabrication process of PVC-diaphragm-based fiber-tip FPI pressure sensor.

and the PVC cap, i.e., surface I, and the other is from the outer surface of the PVC cap, i.e., surface II. The working principle was introduced in Ref. [20].

Fig. 2 schematically illustrates the fabrication process of the PVC-diaphragm-capped FPI, which involves two steps. In step 1, as shown in Fig. 2(a), a section of standard SMF is well cut by a fiber cleaver. In step 2, the multilayer PVC diaphragm is welded to the well-cut end of the SMF by a commercial plastic welder, as illustrated in Fig. 2(b). Using this method, we successfully fabricated a series of solid PVC caps on the end facets of SMFs. Furthermore, the thickness of the PVC cap can be changed by adjusting the layer numbers of the PVC diaphragm.

The reflection spectra and corresponding optical microscope images of the PVC-capped FPI sensors with different cavity lengths of ~ 56 , ~ 47 , ~ 40 , and ~ 17 μm are shown in Fig. 3(a), where it is seen that the free spectral range (FSR) in the reflection spectrum increases with decreasing cavity length. The FSR is given by the Fresnel reflection equation, $FSR = \lambda^2 / (2nL)$, where L is the cavity length, n the refractive index of the cavity, and λ the wavelength. The experimental measured and calculated FSRs are compared at ~ 1330 and ~ 1550 nm, respectively, and the measured FSRs agree well with the calculated values, as shown in Fig. 3(b).

III. PRESSURE RESPONSE AND TEMPERATURE INFLUENCE

An experimental setup, schematically illustrated in Fig. 4, was employed to test the proposed pressure sensor. The setup features a broadband light source (BBS) and an optical spectrum analyzer (OSA) (Model AQ6370C, Yokogawa Electric Corp., Tokyo, Japan) with a resolution of 0.5 nm connected to the other end of the SMF via a 3-dB coupler for the reflection spectrum measurements. A PVC-capped FPI with a cavity length of

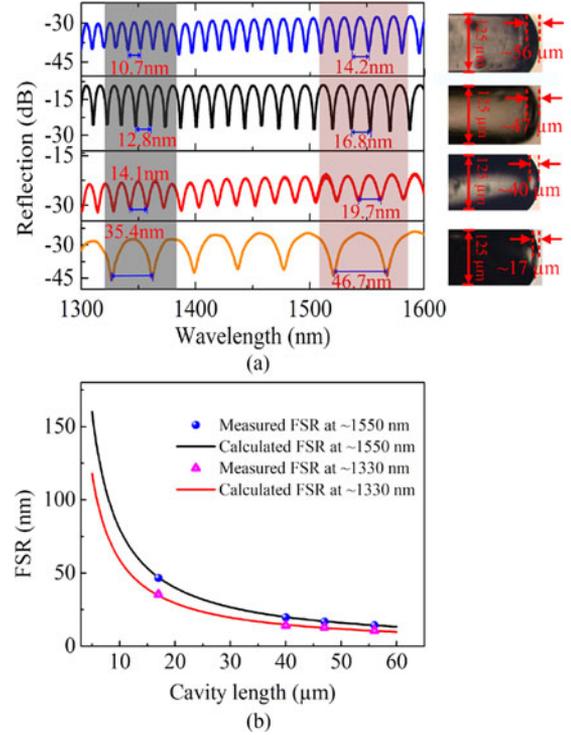


Fig. 3. (a) Reflection spectra and the corresponding microscope images of the four FPIs with different cavity lengths in air at room temperature. (b) Measured and calculated FSRs of the four FPIs at ~ 1330 and ~ 1550 nm, respectively.

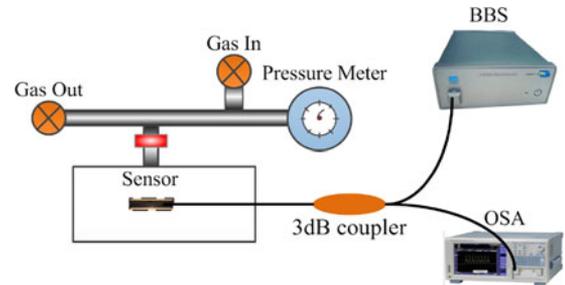


Fig. 4. Experimental setup for pressure measurement.

~ 40 μm was placed into a gas chamber; the chamber employed is the same as that described in [20]. The reflection spectrum of the tested FPI at room temperature (~ 25 $^{\circ}\text{C}$) and standard atmospheric pressure is shown in Fig. 5(a), where the fringe contrast is ~ 15 dB, and the fringe spacing is ~ 21 nm at ~ 1565 nm. The fringe contrast γ can be expressed as [31]

$$\gamma = \frac{2\alpha\sqrt{R_1 R_2 \eta}}{R_1 + R_2 \eta}, \quad (1)$$

which depends on the source coherence α , the intensity ratio of the two reflected light beams, and the transmission coefficient η . The intensity ratio of the two reflected light beams, R_1/R_2 , is determined by the reflectivity of the two interfaces. For the diaphragm-based FPI shown in Fig. 1, the reflectivity of the fiber end/diaphragm interface, R_1 , and that of the diaphragm/air

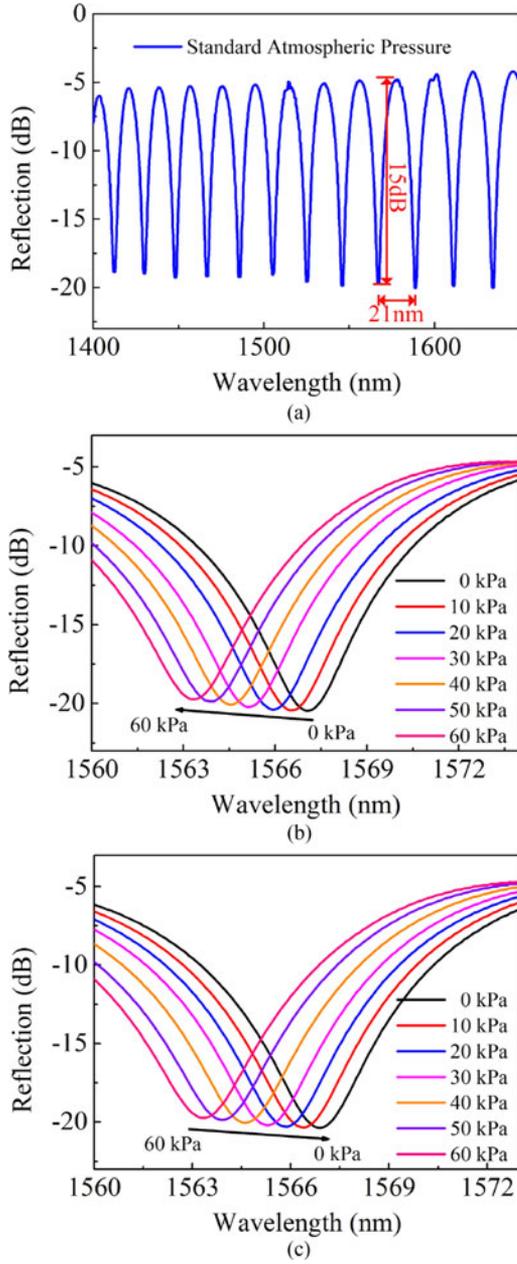


Fig. 5. (a) Reflection spectrum of the FPI with $L = 40 \mu\text{m}$ at standard atmospheric pressure and room temperature. Reflection spectrum evolution of the FPI sensor with (b) an increased gas pressure from 0 to 60 kPa and (c) a decreased pressure from 60 to 0 kPa.

interface, R_2 , is given by

$$R_1 = \frac{(n_1 - n_2)^2}{(n_1 + n_2)^2}, \quad R_2 = \frac{(n_2 - n_3)^2}{(n_2 + n_3)^2}, \quad (2)$$

where n_1 , n_2 , and n_3 are the refractive indices of the fiber, of the diaphragm, and of the air, respectively. The maximum fringe visibility γ can be achieved for the condition $R_1 = \eta R_2$. For the FPI with long cavity length, high reflectivity R_2 is necessary to compensate the loss caused by the decreased transmission coefficient. In our configuration ($n_1 = 1.446$, $n_2 \approx 1.53$, $n_3 = 0$), R_2 is higher than R_1 according to (2), which results in a high fringe

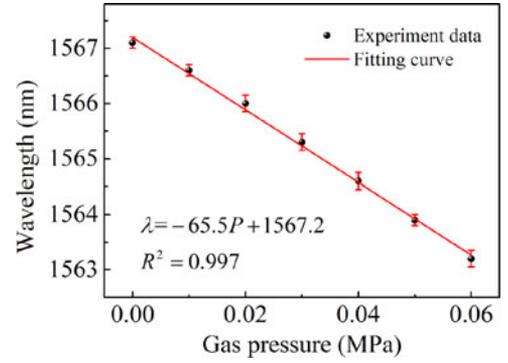


Fig. 6. Wavelength of the tracked dip vs gas pressure.

TABLE I
GAS-PRESSURE SENSITIVITY OF SEVERAL FIBER-OPTIC FPI STRUCTURES

FPI structure	Wavelength sensitivity
FPI embedded in pressure fittings [25]	0.24 nm/MPa
Fiber-tip air-bubble FPI [20]	1.06 nm/MPa
Pendant polymer droplet-based FPI [24]	1.13 nm/MPa
FPI based on concave well on fiber end [26]	1.53 nm/MPa
FPI with open cavity [27]	2.46 nm/MPa
FPI based on dual capillaries [28]	4.15 nm/MPa
Hollow-core photonic bandgap fiber with a side opened channel FPI [29]	4.24 nm/MPa
PVC diaphragm-based FPI (present work)	65.5 nm/MPa

contrast. Moreover, owing to the low reflectivity R_1 , the average reflection level seems to be larger than -10 dB.

The chamber pressure is increased from 0 to 60 kPa in increments of 10 kPa, remaining at each step for 5 min. Resonant dips at approximately 1565 nm are tracked, as shown in Fig. 5(b), where the fringe dip shifts toward shorter wavelength with pressure increasing. Then, the applied pressure is decreased from 60 to 0 kPa, and the tracked dip shifts back to longer wavelength, as shown in Fig. 5(c). The gas pressure is increased and decreased five times and the error-bar charts is provided to illustrate the measurement repeatability. The wavelength of fringe dip versus the applied pressure is illustrated in Fig. 6, where a linear fitting yields an ultrahigh-pressure sensitivity of -65.5 nm/MPa. It is worth noting that the linear response of the sensor can be only achieved in a small pressure range. Due to the mechanical property of the PVC diaphragm, the sensor will present a non-linear response to gas pressure in a large measurement range. A variety of reported fiber-optic FPI gas-pressure sensors that employed different cavity structures are presented in Table I, where the proposed PVC diaphragm-based fiber-tip pressure sensor exhibits the highest sensitivity. The pressure response of the sensor is expressed as

$$\frac{d\lambda}{dP} = \lambda \left(\frac{1}{L} \frac{dL}{dP} + \frac{1}{n} \frac{dn}{dP} \right), \quad (3)$$

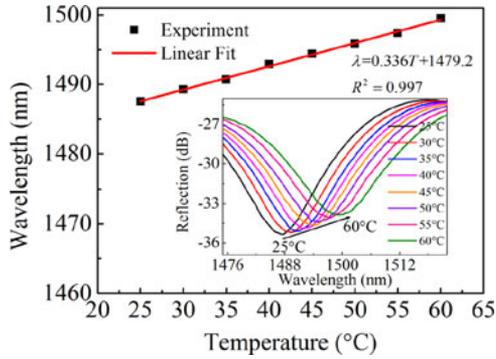


Fig. 7. Wavelength of the fringe dip at ~ 1500 nm vs applied temperature. Inset: reflection spectral evolution from 25 to 60 °C.

where n is the refractive index of the PVC cavity, L the cavity length, P the applied pressure, and λ the wavelength of the interference dips. Since the low elastic modulus of PVC material, dL/dP , can be large, a high pressure sensitivity results. The “blue shift” of the tracked dip with increasing pressure can be explained by both cavity deformation and the refractive-index change of the cavity medium. In the pressure test, it is known that dL/dP is negative and dn/dP is positive, and therefore we believe that the cavity deformation plays a major role in the pressure response of the sensor. The diaphragm we employed is a compound comprised of PVC and some unknown plasticizers, and its elasto-optic coefficient and elastic modulus cannot be assigned, so the quantitative analysis is not given here.

The temperature-induced measurement error was investigated by placing the device in an electrical oven with a temperature stability of ± 0.2 °C. The measurement method has been described in [6] and [30]. The reflection spectral evolution from 25 to 60 °C is illustrated in the inset of Fig. 7, where a red shift is clearly observed with increasing temperature. The shift of the dip wavelength at ~ 1490 nm with increasing temperature is also shown in Fig. 7, where a linear fitting yields a temperature sensitivity of ~ 366 pm/°C. We believe that the temperature drift of the fiber sensor is a result of thermal expansion and thermo-optic effects of the PVC cap according to

$$\frac{d\lambda}{dT} = \lambda \left(\frac{1}{L} \frac{dL}{dT} + \frac{1}{n} \frac{dn}{dT} \right). \quad (4)$$

When no temperature compensation is employed, the error resulting from temperature cross-sensitivity is ~ -5.5 kPa/°C, which is $\sim 40 \times$ lower than that in our previous work [24].

IV. CONCLUSION

We have experimentally demonstrated a novel method of fabricating a PVC diaphragm-based fiber-tip FPI for gas-pressure measurements. The proposed sensor exhibits an ultrahigh gas-pressure sensitivity of -65.5 nm/MPa at ~ 1565 nm and a small temperature cross-sensitivity of ~ -5.5 kPa/°C. The fabrication method is highly efficient, low cost, and repeatable, and employs only a plastic welder and a piece of PVC diaphragm. Owing to advantages of high sensitivity, simple structure, and

good repeatability, the micron PVC diaphragm-based fiber-tip FPI sensor is attractive for pressure monitoring in practical applications.

REFERENCES

- [1] Q. Shi *et al.*, “Environmentally stable Fabry–Pérot-type strain sensor based on hollow-core photonic bandgap fiber,” *IEEE Photon. Technol. Lett.*, vol. 20, no. 4, pp. 237–239, Jan./Feb. 2008.
- [2] J.-R. Zhao, X.-G. Huang, W.-X. He, and J.-H. Chen, “High-resolution and temperature-insensitive fiber optic refractive index sensor based on Fresnel reflection modulated by Fabry–Pérot interference,” *J. Lightw. Technol.*, vol. 28, no. 19, pp. 2799–2803, Oct. 2010.
- [3] M. S. Ferreira, L. Coelho, K. Schuster, J. Kobelke, J. L. Santos, and O. Frazão, “Fabry–Pérot cavity based on a diaphragm-free hollow-core silica tube,” *Opt. Lett.*, vol. 36, pp. 4029–4031, 2011.
- [4] J. Ma, W. Jin, H. Xuan, C. Wang, and H. L. Ho, “Fiber-optic ferrule-top nanomechanical resonator with multilayer graphene film,” *Opt. Lett.*, vol. 39, pp. 4769–4772, 2014.
- [5] M. Li, Y. Liu, R. Gao, Y. Li, X. Zhao, and S. Qu, “Ultracompact fiber sensor tip based on liquid polymer-filled Fabry–Pérot cavity with high temperature sensitivity,” *Sens. Actuators B, Chem.*, vol. 233, pp. 496–501, 2016.
- [6] K. Yang *et al.*, “Ultrasensitive temperature sensor based on a fiber Fabry–Pérot interferometer created in a mercury-filled silica tube,” *IEEE Photon. J.*, vol. 7, no. 6, Dec. 2015, Art. no. 6803509.
- [7] Y. J. Rao, M. Deng, T. Zhu, and H. Li, “In-line Fabry–Pérot etalons based on hollow-core photonic bandgap fibers for high-temperature applications,” *J. Lightw. Technol.*, vol. 27, no. 19, pp. 4360–4365, Oct. 2009.
- [8] X.-H. Fu, H.-Y. Xie, F. Wang, P. Jiang, G.-W. Fu, and W.-H. Bi, “Miniature Fabry–Pérot interferometric sensor for temperature measurement based on photonic crystal fiber,” *Optoelectron. Lett.*, vol. 11, pp. 382–385, 2015.
- [9] H. Bae and M. Yu, “Miniature Fabry–Pérot pressure sensor created by using UV-molding process with an optical fiber based mold,” *Opt. Express*, vol. 20, pp. 14573–14583, 2012.
- [10] W. Wang, N. Wu, Y. Tian, C. Niezrecki, and X. Wang, “Miniature all-silica optical fiber pressure sensor with an ultrathin uniform diaphragm,” *Opt. Express*, vol. 18, pp. 9006–9014, 2010.
- [11] Y. Zhu, K. L. Cooper, G. R. Pickrell, and A. Wang, “High-temperature fiber-tip pressure sensor,” *J. Lightw. Technol.*, vol. 24, no. 2, pp. 861–869, Feb. 2006.
- [12] F. Xu *et al.*, “High-sensitivity Fabry–Pérot interferometric pressure sensor based on a nanothick silver diaphragm,” *Opt. Lett.*, vol. 37, pp. 133–135, 2012.
- [13] Y. Wang, D. Wang, C. Wang, and T. Hu, “Compressible fiber optic micro-Fabry–Pérot cavity with ultra-high pressure sensitivity,” *Opt. Express*, vol. 21, pp. 14084–14089, 2013.
- [14] J. Ma, J. Ju, L. Jin, and W. Jin, “A compact fiber-tip micro-cavity sensor for high-pressure measurement,” *IEEE Photon. Technol. Lett.*, vol. 23, no. 21, pp. 1561–1563, Nov. 2011.
- [15] J. Ma, W. Jin, H. L. Ho, and J. Y. Dai, “High-sensitivity fiber-tip pressure sensor with graphene diaphragm,” *Opt. Lett.*, vol. 37, pp. 2493–2495, 2012.
- [16] L. Chen, C. Chan, W. Yuan, S. Goh, and J. Sun, “High performance chitosan diaphragm-based fiber-optic acoustic sensor,” *Sens. Actuators A, Phys.*, vol. 163, pp. 42–47, 2010.
- [17] J. Xu, X. Wang, K. L. Cooper, and A. Wang, “Miniature all-silica fiber optic pressure and acoustic sensors,” *Opt. Lett.*, vol. 30, pp. 3269–3271, 2005.
- [18] L. Liu *et al.*, “UV adhesive diaphragm-based FPI sensor for very-low-frequency acoustic sensing,” *IEEE Photon. J.*, vol. 8, no. 1, Feb. 2016, Art. no. 6800709.
- [19] H. Bae, D. Yun, H. Liu, D. A. Olson, and M. Yu, “Hybrid miniature Fabry–Pérot sensor with dual optical cavities for simultaneous pressure and temperature measurements,” *J. Lightw. Technol.*, vol. 32, no. 8, pp. 1585–1593, Apr. 2014.
- [20] C. Liao *et al.*, “Sub-micron silica diaphragm-based fiber-tip Fabry–Pérot interferometer for pressure measurement,” *Opt. Lett.*, vol. 39, pp. 2827–2830, 2014.
- [21] K. Totsu, Y. Haga, and M. Esashi, “Ultra-miniature fiber-optic pressure sensor using white light interferometry,” *J. Micromech. Microeng.*, vol. 15, pp. 71–75, 2004.
- [22] G. Hill *et al.*, “SU-8 MEMS Fabry–Pérot pressure sensor,” *Sens. Actuators A, Phys.*, vol. 138, pp. 52–62, 2007.

- [23] E. Cibula and D. Donlagic, "Miniature fiber-optic pressure sensor with a polymer diaphragm," *Appl. Opt.*, vol. 44, pp. 2736–2744, May 2005.
- [24] B. Sun *et al.*, "Simultaneous measurement of pressure and temperature by employing Fabry–Perot interferometer based on pendant polymer droplet," *Opt. Express*, vol. 23, pp. 1906–1911, 2015.
- [25] G. Z. Xiao, A. Adnet, Z. Zhang, Z. Lu, and C. P. Grover, "Fiber-optic Fabry–Perot interferometric gas-pressure sensors embedded in pressure fittings," *Microw. Opt. Technol. Lett.*, vol. 42, pp. 486–489, 2004.
- [26] R. Wang and X. Qiao, "Intrinsic Fabry–Pérot interferometer based on concave well on fiber end," *IEEE Photon. Technol. Lett.*, vol. 26, no. 14, pp. 1430–1433, Jul. 2014.
- [27] R. Wang and X. Qiao, "Gas refractometer based on optical fiber extrinsic Fabry–Perot interferometer with open cavity," *IEEE Photon. Technol. Lett.*, vol. 27, no. 3, pp. 245–248, Feb. 2015.
- [28] B. Xu, C. Wang, D. Wang, Y. Liu, and Y. Li, "Fiber-tip gas pressure sensor based on dual capillaries," *Opt. Express*, vol. 23, pp. 23484–23492, 2015.
- [29] J. Tang *et al.*, "High-sensitivity gas pressure sensor based on Fabry–Pérot interferometer with a side-opened channel in hollow-core photonic bandgap fiber," *IEEE Photon. J.*, vol. 7, no. 6, Dec. 2015, Art. no. 6803307.
- [30] J. Zhou *et al.*, "Simultaneous measurement of strain and temperature by employing fiber Mach-Zehnder interferometer," *Opt. Express*, vol. 22, pp. 1680–1686, 2014.
- [31] J. Ma, "Miniature fiber-tip Fabry–Perot interferometric sensors for pressure and acoustic detection," Ph.D. thesis, Dept. of EE, PolyU, Hong Kong, China, 2014.

Zhe Zhang was born in Pingdingshan, China, in 1992. He received the B.Sc. degree in physics from Huanghuai University, Zhumadian, China, in 2010. He is currently working toward the doctoral degree in the Key Laboratory of Optoelectronic Devices and Systems, Ministry of Education and Guangdong Province, College of Optoelectronic Engineering, Shenzhen University, Shenzhen, China. His current research interests focus on hollow-core photonic bandgap fiber grating sensors, fiber Bragg gratings, and femtosecond laser micromachining.

Changrui Liao received the B.Eng. degree in optical engineering and the M.S. degree in physical electronics from Huazhong University of Science and Technology, Wuhan, China, in 2005 and 2007, respectively, and the Ph.D. degree in electrical engineering from the Hong Kong Polytechnic University, Hong Kong, in 2012. He is currently with Shenzhen University, Shenzhen, China, as an Associate Professor. His current research interests focus on optical fiber sensors and femtosecond laser micromachining.

Jian Tang is a Postdoctoral Research Fellow in the Key Laboratory of Optoelectronic Devices and Systems, Ministry of Education and Guangdong Province, College of Optoelectronic Engineering, Shenzhen University, Shenzhen, China. His current research interests include long-period fiber gratings and air pressure sensors.

Zhiyong Bai received the B.S. degree in physics from Ningbo University, Ningbo, China, in 2008, the M.S. degree in optics from South China Normal University, Guangzhou, China, in 2011, and the Ph.D. degree in optics in Nankai University, Tianjin, China, in 2014. From 2014 to 2015, he was with the State Grid Electric Power Research Institute as an R&D Engineer. Since 2015, he has been a Postdoctoral Research Fellow in the Guangdong and Hong Kong Joint Research Centre for Optical Fiber Sensors, Shenzhen University, China. His current research interests include optical fiber gratings, orbital angular momentum, and optical fiber sensors. He is the author or coauthor of more than 30 journal papers.

Kuikui Guo received the B.S. degree in Photoelectric Information Institute, Changchun University of Science and Technology, Changchun, China, in 2013. He is currently working toward the Ph.D. degree in optical engineering in Shenzhen University, Shenzhen, China. From 2013 to 2015, he was an Optical Engineer in Accu-Tech Co., Ltd, Beijing. His current research interests include optical fiber laser sensors and fiber Bragg gratings.

Maoxiang Hou received the B.Sc. degree in applied physics from Northeastern University, Shenyang, China, in 2011, and the Ph.D. degree in optics from the School of Physics, Huazhong University of Science and Technology, Wuhan, China, in 2016. He is currently a Postdoctoral Researcher in Shenzhen University. His main research interests include optical fiber sensing, photonic crystal-fiber and devices and femtosecond laser micromachining.

Jun He was born in Hubei, China, in 1985. He received the B.Eng. degree in electronic science and technology from Wuhan University, Wuhan, China, in 2006 and the Ph.D. degree in electrical engineering from the Institute of Semiconductors, Chinese Academy of Sciences, Beijing, China, in 2011. From 2011 to 2013, he was with Huawei Technologies, Shenzhen, China, as a Research Engineer. From 2013 to 2015, he was with Shenzhen University, Shenzhen, China, as a Postdoctoral Research Fellow. From 2015 to 2016, he was with The University of New South Wales, Sydney, Australia, as a Visiting Fellow. Since 2017, he has been in Shenzhen University, Shenzhen, China, as an Assistant Professor. His current research interests focus on optical fiber sensors, fiber Bragg gratings, and fiber lasers. He has authored or coauthored 4 patent applications and more than 50 journal and conference papers. He is a member of the Optical Society of America.

Ying Wang, received the B.Sc. degree in applied physics, and the Ph.D. degree in physical electronics from Huazhong University of Science and Technology, Wuhan, China, in 2004 and 2010, respectively. He was with the Department of Electrical Engineering, The Hong Kong Polytechnic University, Hong Kong, as a Research Associate from 2010 to 2015, and joined the College of Optoelectronic Engineering, Shenzhen University, as a Lecturer in 2015. His research interests are optical fiber sensors and femtosecond laser micromachining.

Shen Liu received the Bachelor's degree in electronic information engineering from the Air Force First Aviation College, in 2008, and the Master's degree in circuit and systems engineering from Chongqing University of Posts and Telecommunications, Chongqing, China, in 2013, and the Ph.D. degree in optical engineering from Shenzhen University, Shenzhen, China, in 2017.

Feng Zhang, received the B.S. degree in applied physics from Yantai University, Yantai, China, in 2006, and the M.S. and Ph.D. degrees in condensed matter physics from Beihang University, Beijing, China, in 2010 and 2015, respectively. His doctoral dissertation research was conducted in the area of the luminescence of rare-earth ion doped glasses. Since 2013, he is a Postdoctoral Research Fellow in the Key Laboratory of Optoelectronic Devices and Systems, Ministry of Education and Guangdong Province, College of Optoelectronic Engineering, Shenzhen University, Shenzhen, China. His current research interests include optical fiber sensors and photonic crystal fiber devices.

Yiping Wang was born in Chongqing, China, on July 1, 1971. He received the B.S. degree in precision instrument engineering from Xi'an Institute of Technology, Xi'an, China, in 1995, and the M.S. degree in precision instrument and mechanism and the Ph.D. degree in optical engineering from Chongqing University, China, in 2000 and 2003, respectively, where he received the prestigious award The National Excellent Doctoral Dissertations of China. In 2003, he joined the Department of Electronics Engineering, Shanghai Jiao Tong University, China, as a Postdoctoral Research Fellow and an Associate Professor. In 2005, he joined the Department of Electrical Engineering, Hong Kong Polytechnic University, Hong Kong, as a Postdoctoral Research Fellow and a Research Fellow. In 2007, he joined the Institute of Photonic Technology, Jena, Germany as a Humboldt Research Fellow. In 2009, he joined the Optoelectronics Research Centre, University of Southampton, U.K., as a Marie Curie Fellow. Since 2012, he has been with the Key Laboratory of Optoelectronic Devices and Systems of Ministry of Education and Guangdong Province, College of Optoelectronic Engineering, Shenzhen University, as a Distinguished Professor and a Pearl River Scholar. His current research interests focus on optical fiber sensors, in-fiber gratings, photonic crystal fibers, and fluid-filling technologies. He has authored or coauthored 1 book, 11 patent applications, and more than 180 journal and conference papers with an SCI citation of more than 1400 times. He is a senior member of the Optical Society of America and the Chinese Optical Society.